AD-A073 092

ARMY MISSILE RESEARCH AND DEVELOPMENT COMMAND REDSTO--ETC F/G 17/8

MINICOMPUTER APPLICATIONS IN AUTOMATED TESTING OF ELECTRO-OPTIC--ETC(U)

MAR 79 R W SCHNEIDER

DRDMI-T-79-38


NL

A07 002

DRDMI-T-79-38

NL

END
DARR
PIRED
9-79
DC

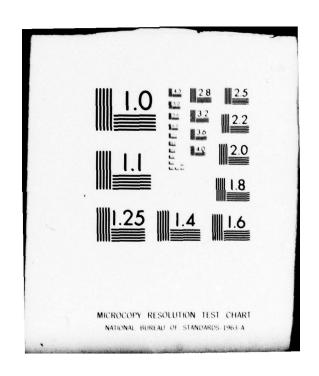



(13)


**TECHNICAL REPORT T-79-38** 

# U.S. ARMY MISSILE RESEARCH AND DEVELOPMENT COMMAND

MINICOMPUTER APPLICATIONS IN AUTO-MATED TESTING OF ELECTRO-OPTICAL GUIDANCE SYSTEMS

Ray W. Schneider
Optical Guidance Technology
Advanced Sensors Directorate
Technology Laboratory

19 March 1979



Approved for Public Release; Distribution Unlimited.

Redstone Arsenal, Alabama 35809

79 08 24 042

### DISPOSITION INSTRUCTIONS

DESTROY THIS REPORT WHEN IT IS NO LONGER NEEDED. DO NOT RETURN IT TO THE ORIGINATOR.

### DISCLAIMER

THE FINDINGS IN THIS REPORT ARE NOT TO BE CONSTRUED AS AN OFFICIAL DEPARTMENT OF THE ARMY POSITION UNLESS SO DESIGNATED BY OTHER AUTHORIZED DOCUMENTS.

### TRADE NAMES

USE OF TRADE NAMES OR MANUFACTURERS IN THIS REPORT DOES NOT CONSTITUTE AN OFFICIAL ENDORSEMENT OR APPROVAL OF THE USE OF SUCH COMMERCIAL HARDWARE OR SOFTWARE.

Unclassified
SECURITY CLASSIFICATION OF THIS PAGE (When Date Entered)

T-7		DOCUMEN ! N	TION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
	ORT NUMBER 9-38	/	2. GOVT AC	CESSION NO.	3. RECIPIENT'S CATALOG NUMBER
	Transfer to the second				5 DYRE OF REPORT & PERIOD COVER
	Minicomputer Applications in Automated Testing of Electro-Optical Guidance Systems		PROPERTY AND ADDRESS OF		
Min			sting	Technical Report	
01			Terelos	6. PERFORMING ORG. REPORT NUMBER	
. AUTH	10R(+)				8. CONTRACT OR GRANT HUMBER(s)
-					
Ray	W./Schneider				
. PERF	FORMING ORGANIZATI	ION NAME AND AC	DORESS		10. PROGRAM ELEMENT PROJECT, TAS
	mander	account and	Davidanment	C	AREA & WORK UNT NUMBERS
ATTI	Army Missile R N: DRSMI-TE			Command	11) Laprop.
	stone Arsenal,		35809		12. EPORT DATE
Com	mander				19 Mar 79
	Army Missile R		Development	Command	13. NUMBER OF PAGES
Red	N: DRSMI-TI stone Arsenal. HTORING AGENCY NA	Alabama	35809	line Office)	15. SECURITY CLASS, (of this report)
	_	and the second second second	per appropriate and the second second second second	Table of the last	Unclassified
,	WIDOD	MIT	7-79-35	31	
(	THINK	(V)	A CONTRACTOR OF THE PROPERTY O	mounts.	154. DECLASSIFICATION/DOWNGRADING
6. DIST	RIBUTION STATEMEN	IT (of this Report)			
7. DIST	RIBUTION STATEMEN	IT (of the abstract	entered in Block 20,	il different from	n Report)
O. SUPI	PLEMENTARY NOTES				
. KEY	WORDS (Continue on re	reces side il neces	eeary and identify by	block number)	
ALSPES AUTOMAT		AUTOMAT	ED TESTING		
	Caalcan		MINICOM	PUTER APPLICATIONS	
	lse Repetition	Frequency	(prf)		
Pu	FRACT (Continue on Per			lock number)	
					System (ALSPES) has been

393 427

SECURITY CLASSIFICATION OF THIS PAGE(When Date Entered)

are fed into a CRT terminal and the minicomputer conducts a fully automated, hands-off test by varying such parameters as laser energy, target position and velocity, seeker position and angular rate, and time separation between targets. This report discusses the types of automated tests performed, the electro-optical test equipment utilized and the layout of the test facility, the minicomputer to test equipment interface, and the cost savings resulting from the development of this automated test facility.

Unclassified

SECURITY CLASSIFICATION OF THIS PAGE(When Date Entered

# **ACKNOWLEDGMENTS**

The Author wishes to thank Mr. E. Doug Crosswhite for helpful discussions in the planning and operation of the ALSPES facility, and the local Sperry Support Services group for timely delivery of critical components which they fabricated as required by Contract DAAK40-77-C-0034.

	sion For	
NTIS		
DDC TA	AB.	0
Unanno	unced	
Justif	cication	
Ву		
Dietni	hution/	
Distri	bution/	
	bution/ ability	Codes
	ability	
Avail	ability Availan	d/or
	ability	d/or
Avail	ability Availan	d/or
_Avail	ability Availan	d/or

# CONTENTS

Section	ion	Page
1.	Introduction	
2.	Facility Description	3
	A. Data Processing System	
	B. Darkroom	5
3.	Software	6
4.	Conclusions	7

# ILLUSTRATIONS

Figur	e Page
1.	Laser Dynamic Range Simulation Facility 9
2.	Block Diagram of Minicomputer to Control Function Interface for
	Automated Laser Seeker Performance Evaluation System (ALSPES)10
3.	ALSPES Data and Control Flow Diagram
4.	Programming Station and Test Control Function Area Outside Seeker
	Test Enclosure
5.	Room Layout of MIRADCOM ALSPES Facility
6.	Laser Sources, Energy Monitor, Neutral Density (ND) Filter Boxes, and
	Two-Axis Beam Scanner Mounted on Isolation Table
7.	Laser, Filter Box, Scanning Mirror, and Diffusing Screen Layout
8.	Solenoid Activated ND Filter Box
9.	Seeker Two-Axis Rate Table

### 1. INTRODUCTION

Since the early development (about 10 years ago) of laser seekers for missile and projectile terminal guidance applications, the US Army Missile Research and Development Command (USAMIRAD-COM) has been involved in the performance evaluation of these seekers using laboratory test facilities. The Advanced Sensors Directorate (AdSeD) of USAMIRAD-COM is responsible for evaluating the seeker design of major terminal guidance missile and projectile systems, identifying seeker problem areas, and making recommendations for their solution. Until the development of the Automated Laser Seeker Performance Evaluation System (ALSPES) described herein, conducting the series of tests required to fully evaluate the seeker performance, specification compliance, and identification of problem areas was a time-consuming task requiring about three days with two people full-time. The types of tests required to fully characterize the seeker are shown in Table 1 with typical times required for completion by both old test techniques and ALSPES. Listed below is a test report\* describing in detail the procedures and test results on a semi-active laser seeker tested according to the conventional, pre-ALSPES test techniques. The user times listed for ASLPES are based on our experience with the facility during the past several months since its completion.

### 2. FACILITY DESCRIPTION

Figure 1 shows the conventional facility used to conduct seeker performance evaluations. It consists of a laser with means of varying the laser energy (neutral density filter box), a set of mirrors to simulate laser target motion on the diffusing screen, and a three degree-of-freedom table on which the seeker is mounted. From the list of tests shown in Table 1, one can see that the control functions which have to be driven in order to conduct the performance evaluation are, as minimum, variation in laser energy, x/y mirror position, pitch/yaw table position, laser turn on/turn off, seeker input/output (I/O) functions, and time separations between multiple laser pulses. Before development of ALSPES, these functions had to be independently controlled by hand from control consoles during each test. The use of a minicomputer to implement these control functions in the construction of the ALSPES facility has greatly reduced the amount of time consumed to generate the required test data.

### A. DATA PROCESSING SYSTEM

Figure 2 shows a block diagram of the HP2174A general purpose and expandable

<sup>\*</sup>Test Report, Laboratory Performance Evaluation of Army SM712 Copperhead B016/2 Laser Seeker (U), Technical Report T-78-68 dated 21 July 1978, MIRADCOM (confidential).

TABLE 1. LASER SEEKER PERFORMANCE TESTS AND TIME SAVINGS ACHIEVABLE WITH AUTOMATED TEST FACILITY (ALSPES)

Test Test	Time Conventional	Time ALSPES
Sensitivity	1 hr	1/2 hr
Boresight Shift with Range Closure	1 hr	1/2 hr
Proportional Zone	2 hrs	1/2 hr
Instantaneous Field-of-View (IFOV)	2 hrs	1/2 hr
Optical Gimbal Coupling (OGC)	2 hrs	1 hr
Maximum Gyro Slew Rate	2 hrs	1 hr
Gyro Dynamics with Target Step LOS Change	2 hrs	1 hr
Gimbal Angle Output Linearity	1 hr	1/2 hr
Correlation/Decorrelation Logic	1 hr	1/2 hr
False Target Ambiguity Discrimination	10 hrs	4 hrs
Total	24 hrs	10 hrs

control and data acquisition system being provided for the ALSPES project. The 20-kHz analog-to-digital (A/D) interface subsystem provides for up to 16 analog inputs, and the HP91063A digital I/O subsystem provides sufficient interfaces to all instruments, mounts, and seekers.

The ALSPES data and control flow diagram in *Figure 3* illustrates the flow of test data and feedback data and the manual and computer signal flow to the test equipment.

The digital I/O subsystem and analog input options interface to the various seekers through "personality" modules. The digital I/O also operates control electronics for the variable optical filters, pulse delay generators, mirror galvanometers, and table position. Radiation measurements are input to the computer through the analog inputs.

The 2113 CPU contains a real-time clock which is used to time-annotate data measurements. The flexible disc is used both for data storage and program storage. The 2645A display station is used to select the test being run and to specify the test parameters and sampling times.

For complete stand-alone operation of the data processing system, a Tektronix Model 4012 Graphics Terminal with Model 4631 Hard Copy Unit is included. These units provide high-speed, computergenerated plots with 1024 by 780 viewable points on a 6.375 x 8.250 in. storage screen.

The hard copy unit can then produce plots of maximum complexity in not more than 18 sec. The HP2174A is designed to interface these Tektronix units through its 12531C interface board in conjunction with the Tektronix Option 06 computer port.

The HP2174A minicomputer, digital I/0 subsystem, and control electronics outside the seeker test enclosure are shown in *Figure* 4.

### B. DARKROOM

The laser seeker test enclosure is a prefabricated structure with wall and ceiling panels of honeycomb construction. The room measures 12 x 28 ft with 8-ft walls. The inside surfaces have been covered with ECCOSORB CV-3 black anechoic foam material which has been measured to have a reflectance of 1.5% or less at the laser wavelength. The floor is covered with black corrugated rubber matting. The layout of the ALSPES darkroom is shown in Figure 5. Three low energy (5 - 10 mJ) Nd:YAG lasers are mounted on top of an airsuspension isolation table with their associated neutral density filter boxes, solenoid activated (NDF/SA). Three lasers in conjunction with a time delay generator system are used to simulate three targets spatially and temporally displaced with respect to each other. In this way a true target, a foreground false target, and a background false target are simulated during a test of the seeker's false target ambiguity discrimination logic. The lasers,

NDF/SA boxes, and scanning mirror on the isolation table are shown in Figure 6, and a top view of the isolation table assembly and diffusing screen is shown in Figure 7. An HE-NE laser is used to optically align the lasers, NDF/SA boxes, and mirror assembly and to visually display target motion on the screen. Figure 8 shows construction details of the NDF/SA box. This filter box has a dynamic range of attenuation of 62.5 dBP and is programmed via the minicomputer to simulate missile or projectile range closure by moving discrete ND filters out of the laser beam as a function of flight time. Eight discrete ND filters are used in the box, the filters having optical densities of 3.2, 1.6, 0.8, 0.4, 0.2, 0.1, 0.05, and 0.025, respectively. Using this combination of filters, the 62.5 dBP range closure can be covered in steps of 0.25 dBP on a pulse-to-pulse basis.

The IR scanner is a galvanometer-type beam deflector utilizing I X I in. mirrors on each axis. The scanner-to-screen distance is set for a 4 x 4 ft screen scan with a beam deflection of ±15 deg. Maximum response of the scanner is 300 deg/sec (15 deg in 5 msec). The mirror servomechanism electronics and Control and Data Acquisition Module (CDAM) to scanner interface package are rack mounted. Specifications for the laser beam scanner are shown in Table 2.

The two-axis rotary table consists of a universal single-axis, mechanical-bearing drive assembly for the yaw axis and a fabricated single-axis, mechanical-bearing slew assembly for the pitch axis. The two-axis rate table inside the seeker test enclosure is shown in *Figure 9*. The drive system for both axes is contained in a single rack mount which accepts a five-digit parallel word command for each axis and generates the serial data necessary to move the drive from its present position to the position specified by the parallel words.

Each axis is capable of 90 ft-lb of peak torque. Reflected inertia is minimized for maximum efficiency. A selectable manual rate and position switch and a 0.1% precision tachometer are included so the yaw axis has full rate table capability. The yaw axis can support up to 2000 lb.

The time delay generator system uses a sync pulse coded to the required laser pulse repetition frequency (prf) to trigger the firings of laser flashlamps and pockels cells for the three lasers. Time delays between the spatially separated lasers are set by delays in flashlamp firings. The pockels cell firing delay from the onset of the flashlamp pulse for each respective laser, is triggered off the flashlamp. In this way each laser's pockels cell is fired at the optimum point during the flashlamp pump.

### 3. SOFTWARE

User programs have been written to exercise the laser beam scanner, two-axis rate table, time delay generators, and solenoid-activated neutral density filter boxes. Missile and projectile range closure

programs driving the NDF/SA boxes are completed; they have the flexibility of simulating any tactical scenario. Software routines have been written and documented for the tests described in *Table 1.\*\** Updates of these tests along with routines for additional tests are continuing.

### 4. CONCLUSIONS

The Advanced Sensors Directorate (AdSeD) of MIRADCOM is responsible for evaluating the seeker design of major terminal guidance missile and projectile systems, identifying seeker problem areas, and making recommendations for their solution. The Automated Laser Seeker Performance Evaluation System (ALSPES) facility described in this paper has given MIRADCOM the capability to conduct

comprehensive performance evaluations of laser seekers in a laboratory environment in a fraction of the time required by old test procedures. The use of a minicomputer in ALSPES to implement control functions such as laser energy variation, seeker position, and target location coupled with the automated printout and plotting of the seeker I/O test parameters during the particular test run has resulted in a "handsoff" environment such that total test time is now approximately 40% of the previously required time. In addition, the facility has enabled AdSeD to conduct a more complete and comprehensive identification of potential seeker problem areas than has been possible heretofore, resulting in an increase in the number of electro-optical terminal guidance seeker design change recommendations to the system developer.

<sup>\*\*</sup>COPPERHEAD Test Programs Operations Manual, SP-220-1046, Sperry Support Services, 30 September 1978.

## TABLE 2. SPECIFICATIONS FOR TAI 2-AXIS LASER BEAM SCANNER

Beam Deflection
Response to 40-Deg Step 6m
Input
Input Impedance
Beam Deflection Gain Factor
Linearity 0.1% F
Optical Transmittance at Laser Wavelength
Intensity Variation at Scanned Spot
Power Amplifier Fuses

±20 Degrees
6mS, X-Axis, 7mS, Y-Axis
±10 Volts
60K Ohms
2 Degrees/Volt
0.1% Peak-to-Peak Excursion
TBD
63.75 dBP

1A 3AG

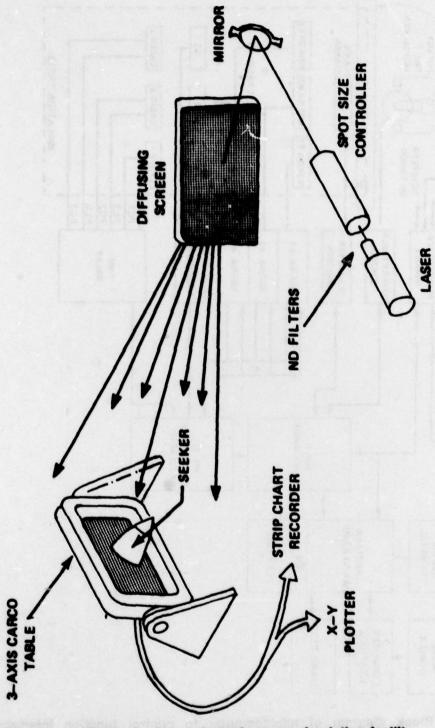


Figure 1. Laser dynamic range simulation facility.

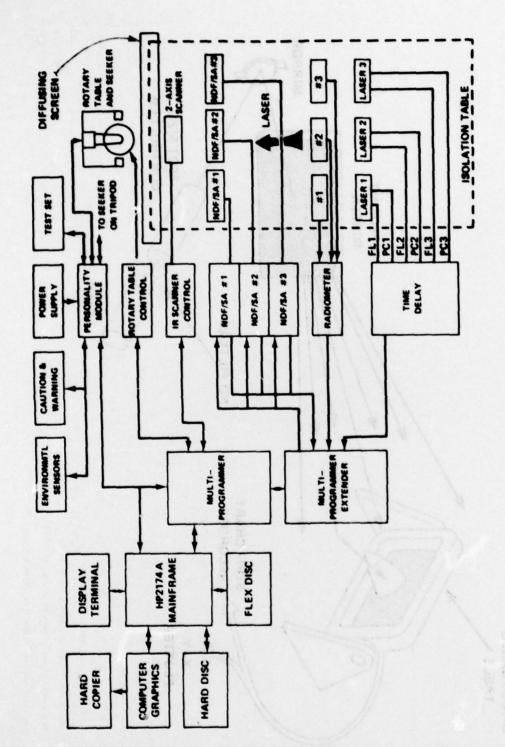


Figure 2. Block diagram of minicomputer to control function interface for Automated Laser Seeker Performance Evaluation System (ALSPES).

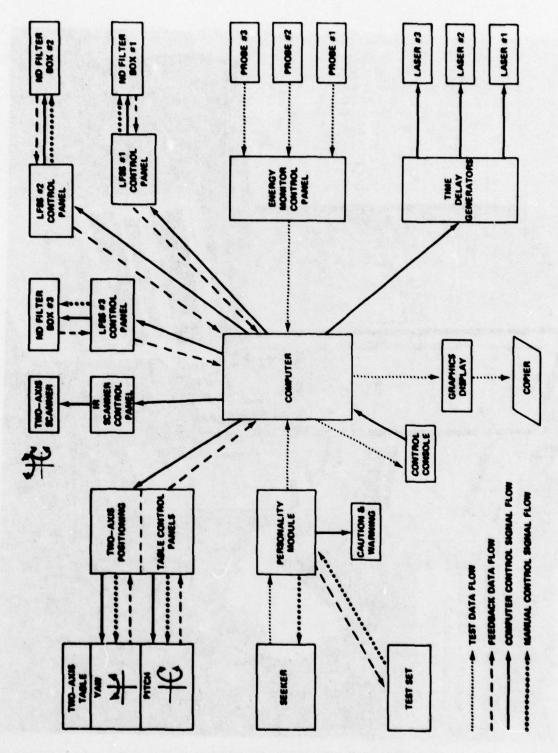


Figure 3. ALSPES data and control flow diagram.


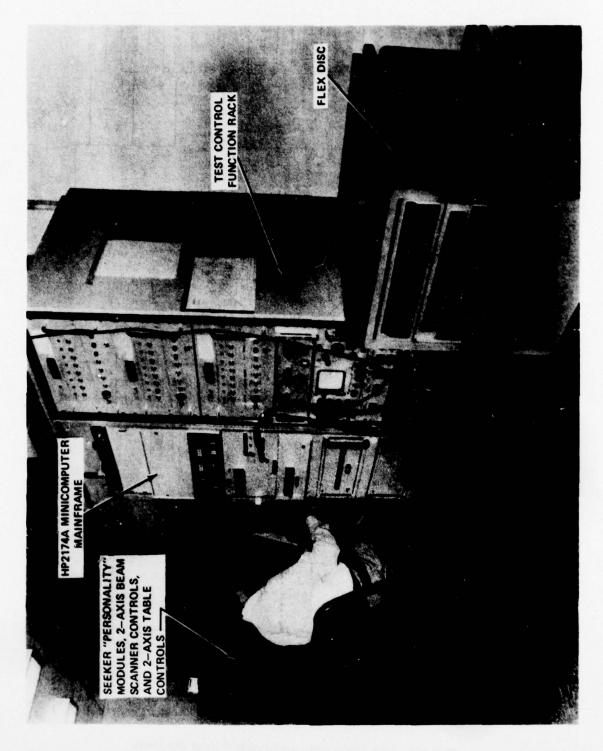


Figure 4. Programming station and test control function area outside seeker test enclosure.

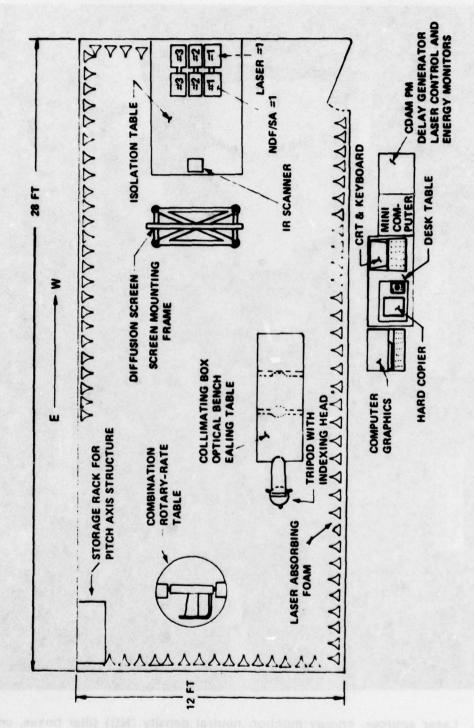

The state of the s

Figure 5. Room layout of MIRADCOM ALSPES facility.

The same of the sa

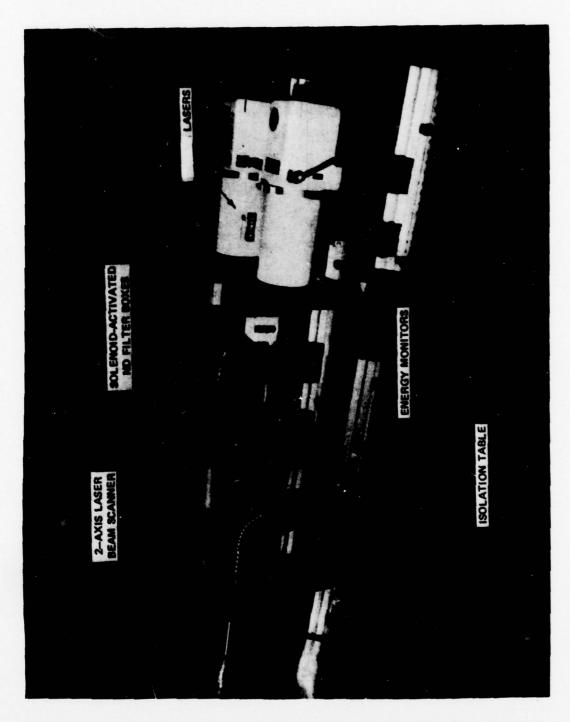


Figure 6. Laser sources, energy monitor, neutral density (ND) filter boxes, and two-axis beam scanner mounted on isolation table.

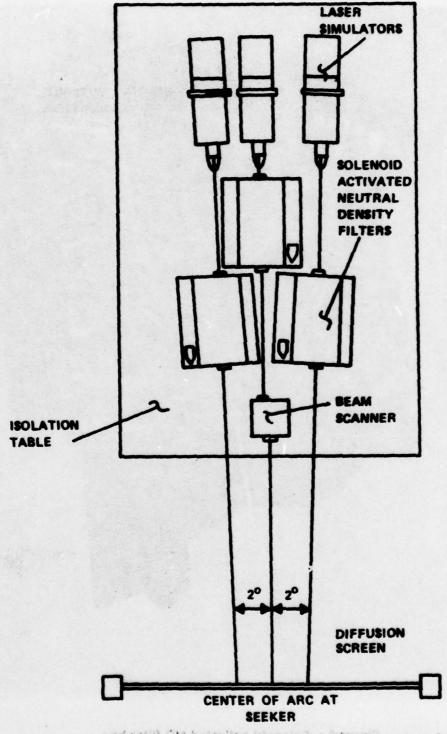


Figure 7. Laser, filter box, scanning mirror, and diffusing screen layout.

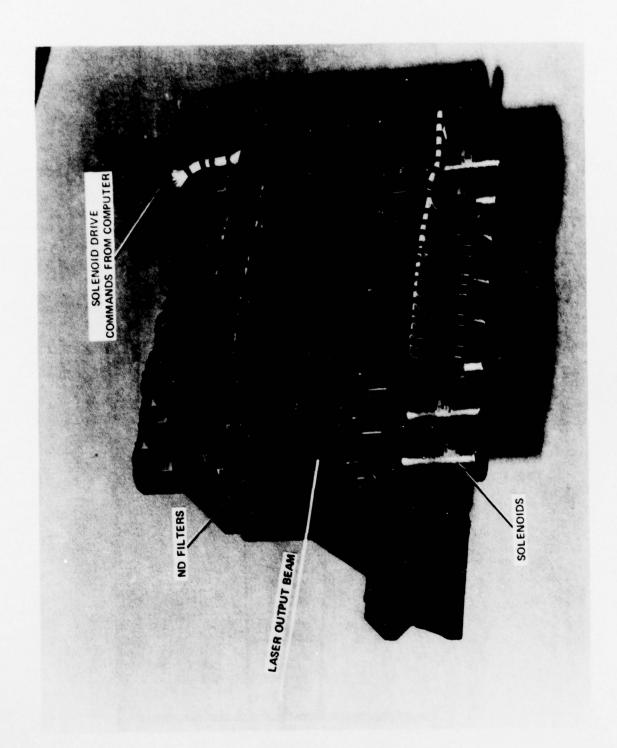


Figure 8. Solenoid activated ND filter box.

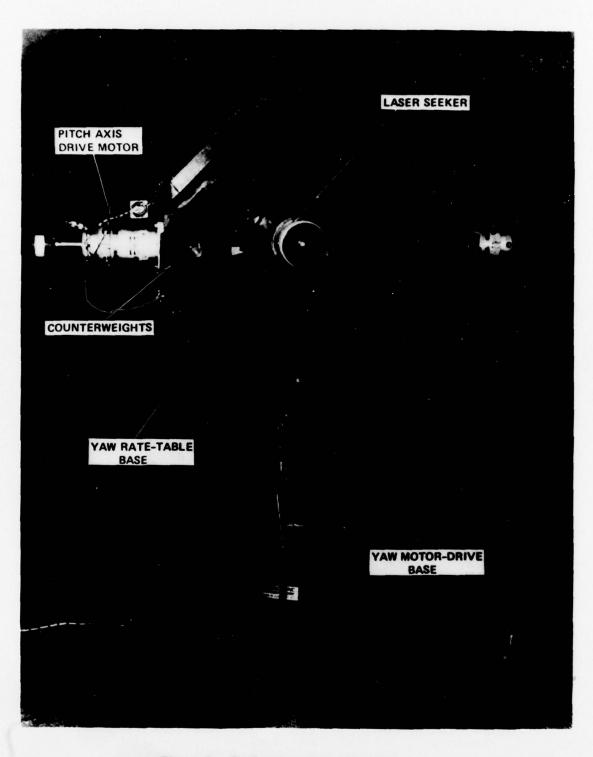


Figure 9. Seeker two-axis rate table.

# DISTRIBUTION

	No. of	No	o. of
C	opies	Col	pies
Defense Documentation Center		Headquarters	
Cameron Station	12	Department of the Army	
Alexandria, Virginia 22314		ATTN: DDCSRDA (DAMA-CSM), LTC C. Jones	1
IIT Research Institute		Washington, DC 20310	
ATTN: GACIAC	1	Office, Director of Defense Research and Engineering	0
10 West 35th Street		Department of Defense	
Chicago, Illinois 60616		ATTN: Land Warfare, Dr. Allen	1
		Washington, DC 20310	
Commander		Office, Secretary of Defense	
US Army Materiel Development and Readiness		ATTN: OSDDRE-DDT&E (TST&E) COL Minich	1
Command		Washington, DC 20310	P. Carlo
ATTN: DRCDE-R	1	Washington, DO 20010	
5001 Eisenhower Avenue		Department of the Army	
Alexandria, Virginia 22333		Office of the Under Secretary	
		ATTN: Under Secretary LaBerge	1
		Washington, DC 20310	
Commander			
Missile Electronics Warfare		Deputy Under Secretary of the Army	
ATTN: DRSEL-WLM-ST, Mr. L. Hogue	1	ATTN: SAVS-OR, Dr. Fallen	1
White Sands Missile Range, New Mexico 88002		Room 2E621, Pentagon	
		Washington, DC 20310	
Commander		Assistant Secretary of the Army	
US Army Armament Research and Development		(R&D) Pentagon	
Command		Washington, DC 20310	1
ATTN: DRCPM-CAWS-GP, Mr. E. Manley	1		
Mr. E. Zimpo	1	Commander	
Dover, New Jersey 07801		USAIIC	
		HQDA (MIIC-CO)	1
		Washington, DC 20310	
DRCPM-CAWS-FO, Mr. Clinkenbeard	1		
		Under Secretary of the Army for Operations Research	h
DRSMI-V, MAJ Love	1	ATTN: Mr. D. C. Hardison	.1
		Washington, DC 20310	
DRCPM-HF, COL Pelligrini	1		
-HFE, M. R. Comer	1	Headquarters	
		Department of the Army	
		ATTN: DACA-AME-C	1
DRSMI-T, Dr. J. Kobler	1	DACS-AME-CD	1
DRSMI-TG, Mr. Huff	1	DAMA-AOA-M	1
DRSMI-TGT, Mr. Leonard	1	DAMA-CSC	1
DRSMI-TE, Mr. W. Lindberg	1	DAMA-CSM	1
DRSMI-TEO, Mr. H. Bates	1	DAMA-DDC	1
DRSMI-TEO, Mr. R. Schneider	20		
DRSMI-TED	3	Commander	-
DRSMI-TBD	3	US Army Armament Research and Development	
DRSMI-TI (Reference Copy)	1	Command	
DRSMI-TI (Record Set)	1	ATTN: DRDAR-LCU-T, Mr. D. Ladd	1
videl start	3116-Q	2.12.11.200.11, 21.2.111011013	1
DRSMI-LP, Mr. Voigt	1	Dover, New Jersey 07801	